



# User Manual

Disclaimer: Products are intended for research use only

NEED HELP?



**SHENTEK** **B**iofargo

🌐 [www.biofargo.com](http://www.biofargo.com)  
📞 804-529-2296  
✉️ [contact@biofargo.com](mailto:contact@biofargo.com)

**SHENTEK**

**Residual Hi5&AcNPV DNA  
Quantitation Kit  
User Guide**

Version: A/1  
For Research Use Only  
Product No.: 1101102  
Reagents for 100 Reactions

Biofargo, Inc.

*(IMPORTANT: Please read this document carefully before experiment.)*

## 1. Product information

### ■ Product description

SHENTEK® Residual Hi5&AcNPV DNA Quantitation Kit is used to quantitate residual Hi5&AcNPV host DNA in different stages of biopharmaceutical products, from in-process samples to final products. This kit utilizes multiplex quantitative PCR (qPCR) technique to perform rapid, specific, and reliable quantitation at the femtogram (fg) level. IPC (Internal Positive Control) is included in the assay to evaluate the performance of each PCR reaction. For extraction information, please refer to the SHENTEK® Residual Host Cell DNA Sample Preparation Kit User Guide (Product No. 1104191).

### ■ Kit contents and storage

*WARNING: Please read the Material Safety Data Sheets (MSDSs) and follow the handling instructions. Wear appropriate protective eyewear, mask, clothing and gloves.*

Table 1. Kit components and storage

Reagent	Part No.	Quantity	Storage
Hi5&AcNPV DNA Control	NNA034	lyophilized powder × 1 tube	-20°C
Hi5&AcNPV Primer&Probe MIX	NNC038	300 µL × 1 tube	-20°C, protect from light
qPCR Reaction Buffer	NNB001	850 µL × 2 tubes	
IPC MIX	NNC067	150 µL × 1 tube	
DNA Dilution Buffer (DDB)	NND001	1.5 mL × 3 tubes	-20°C

The kit components can be stored at appropriate conditions for up to 24 months.

Please check the expiration date on the labels.

### ■ Applied instruments, including but not limited to the following

➤ SHENTEK-96S Real-Time PCR System

➤ 7500 Real-Time PCR System

- CFX96 Real-Time PCR System
- FQD-96A Real-Time PCR System


## ■ Required materials not included in the kit

- Nonstick, DNase-free & Low Retention Microfuge Tubes, 1.5 mL
- Nonstick, Low Retention Tips: 1000  $\mu$ L, 100  $\mu$ L and 10  $\mu$ L
- 96-well qPCR plates with sealing film or PCR 8-strip tubes with caps

## ■ Related equipment

- Real-Time PCR System
- Vortex mixer
- Benchtop microcentrifuge
- Micropipettes: 1000  $\mu$ L, 100  $\mu$ L and 10  $\mu$ L
- Microplate shaker

## ■ Workflow

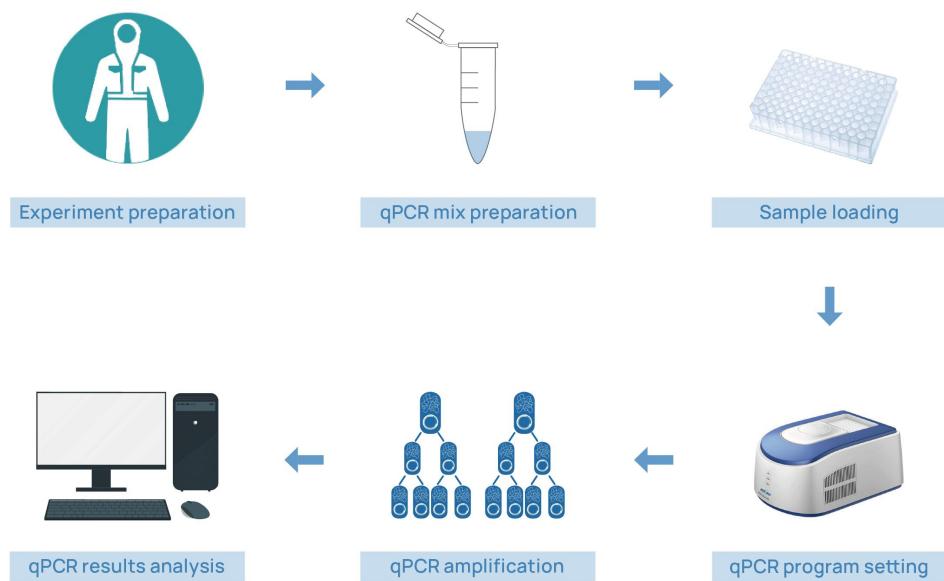

## 2. Methods

### ■ Experiment preparation

1. Wear appropriate protective eyewear, mask, clothing and gloves.
2. Irradiate the tabletop, micropipettes and tubes with UV for 30 minutes, and disinfect with 75% ethanol.
3. Thaw the kit completely at 2-8°C or melt on ice, vortex and spin briefly.

### ■ DNA Control serial dilutions for the standard curve

Please check the concentration labeled on the tube containing the Hi5&AcNPV DNA Control prior to dilution. The concentration of Hi5 DNA control is 30 ng/µL, and AcNPV DNA control is 2 ng/µL (equivalent to  $5.14 \times 10^8$  copies/µL).

1. Quickly spin the Hi5&AcNPV DNA Control for 15 seconds, and add precisely 55 µL of ddH<sub>2</sub>O to the bottom of the tube. Vortex to mix well and quickly spin down the reagents for 10 seconds in microcentrifuge, and repeat 3 times. Let the tube stand for another 10 minutes before use.
2. Label seven nonstick 1.5 mL microfuge tubes: ST, ST0, ST1, ST2, ST3, ST4 and ST5.
3. Dilute the Hi5&AcNPV DNA Control 10-fold with DDB in the ST tube. Vortex to mix well and quickly spin down the reagents for 3-5 seconds in microcentrifuge, and repeat 3 times to mix it thoroughly.
4. Add 90 µL DDB to each tube: ST0, ST1, ST2, ST3, ST4, and ST5.
5. Perform the serial dilutions according to Table 2:

Table 2. Dilution for Hi5&amp;AcNPV DNA Control

Serial dilution tube	Dilution	Hi5 (pg/µL)	AcNPV (copies/µL)*	AcNPV (pg/µL)*
ST0	10 µL ST + 90 µL DDB	300	$5.14 \times 10^6$	20
ST1	10 µL ST0 + 90 µL DDB	30	$5.14 \times 10^5$	2
ST2	10 µL ST1 + 90 µL DDB	3	$5.14 \times 10^4$	0.2
ST3	10 µL ST2 + 90 µL DDB	0.3	$5.14 \times 10^3$	0.02
ST4	10 µL ST3 + 90 µL DDB	0.03	$5.14 \times 10^2$	0.002
ST5	10 µL ST4 + 90 µL DDB	0.003	$5.14 \times 10^1$	0.0002

\*For AcNPV DNA, either copy number concentration or mass concentration can be selected as standard curve.

- The remaining unused DDB need to be stored at 2-8°C. If the solution is cloudy or contains precipitates, heat at 37°C until it clear.
- At least five concentration of standard curve should be included. To select appropriate sample dilutions, we recommend to perform method validation before sample testing.

## ■ Sample preparation

- Negative Control Sample (NCS) Preparation

Add 100 µL of DDB to a new 1.5 mL microfuge tube, and label as NCS.

NCS and samples should be prepared in same way during DNA extraction.

## ■ qPCR MIX preparation

1. Determine the number of reaction wells based on your selected standard curve, with the number of test samples and control samples. Generally, triplicates are tested for each sample.

Number of reaction wells = (5 standard points on the standard curve + 1 NTC + 1 NCS + test samples)×3

2. Prepare qPCR MIX according to the number of reaction wells in Table 3.

Table 3. qPCR MIX Preparation

Reagents	Volume/reaction	Volume for 30 reaction (includes 10% overage)
qPCR Reaction Buffer	15.9 $\mu$ L	524.7 $\mu$ L
Hi5&AcNPV Primer&Probe MIX	2.8 $\mu$ L	92.4 $\mu$ L
IPC MIX	1.3 $\mu$ L	42.9 $\mu$ L
Total volume	20 $\mu$ L	660 $\mu$ L

3. Mix thoroughly and place on ice, aliquot 20  $\mu$ L/well into 96-well qPCR plates or PCR 8-strip tubes.

## ■ qPCR Reaction MIX preparation

1. Prepare qPCR Reaction MIX according to Table 4, and 96-well plate layout is shown in Table 5.

Table 4. qPCR Reaction MIX Preparation

Tubes	Standard curve	NTC	NCS	Test sample
qPCR MIX	20 $\mu$ L	20 $\mu$ L	20 $\mu$ L	20 $\mu$ L
Samples	10 $\mu$ L ST1 - ST5	10 $\mu$ L DDB	10 $\mu$ L purified NCS	10 $\mu$ L purified test sample
Total Volume	30 $\mu$ L	30 $\mu$ L	30 $\mu$ L	30 $\mu$ L

Table 5. Example of 96-well Plate layout

NTC		S1	S1	S1								A
NTC		S2	S2	S2					ST5	ST5	ST5	B
NTC		S3	S3	S3					ST4	ST4	ST4	C
		S4	S4	S4					ST3	ST3	ST3	D
NCS		S5	S5	S5					ST2	ST2	ST2	E
NCS									ST1	ST1	ST1	F
NCS												G
												H
1	2	3	4	5	6	7	8	9	10	11	12	

- This example represents the assay for a standard curve with 5 concentration

*gradients (ST1-ST5), 1 NTC, 1 NCS, and 5 test samples (S1-S5), with 3 replicates for each sample.*

- *In specific testing, the plate layout for sample loading can be adjusted based on the sample quantity. Please refer to the example shown in Table 5.*

2. Seal the 96-well plate with sealing film. Mix well in microplate shaker, then spin down the reagents for 10 seconds in microcentrifuge and place it on the qPCR instrument.

## ■ qPCR program setting

*NOTE: The following instructions apply only to the ABI7500 instrument with SDS v1.4. If you use a different instrument or software, refer to the applicable instrument or software documentation.*

1. Create a new document, then in the Assay drop-down list, select Standard Curve (**Absolute Quantitation**).
2. In the Run Mode drop-down list, select **Standard 7500**, then click **Next**.
3. Click **New Detector**:
  - a. Enter Hi5-DNA in the Name field.
  - b. Select **FAM** in the Reporter Dye drop-down list and select **(none)** in the Quencher Dye drop-down list, then click **OK**.
  - c. Select a color for the detector, then click **Create Another**.
4. Click **New Detector**:
  - d. Enter AcNPV -DNA in the Name field.
  - e. Select **CY5** in the Reporter Dye drop-down list and select **(none)** in the Quencher Dye drop-down list, then click **OK**.
  - f. Select a color for the detector, then click **Create Another**.
5. Click **New Detector**:
  - a. Enter IPC in the Name field.
  - b. Select **VIC** in the Reporter Dye drop-down list and select **(none)** in the Quencher Dye drop-down list, then click **OK**.

- c. Select a color for the detector, then click **OK**.
- d. Select the detectors, then click **Add** to add the detectors to the document.
- 6. Select **ROX** as the passive reference dye, then Click **Next**.
- 7. Select the applicable set of wells for the samples, then select **Hi5-DNA, AcNPV -DNA detector and IPC detector** for each well.
- 8. Select **Finish**, and then set thermal-cycling conditions:
  - a. Set the thermal cycling reaction volume to 30  $\mu$ L.
  - b. Set the temperature and time as follow in Table 6:

Table 6. qPCR running temperature and time

Step	Temp.	Time(mm:sec)	Cycles
Activation	95°C	10:00	1
Denaturation	95°C	00:15	40
Annealing/extension	60°C*	1:00	

\*Instrument will read the fluorescence signal during this step.

- 9. Save the document, then click **Start** to start the real-time qPCR run.

## ■ Results analysis

1. Select **Set up** tab, then set tasks for each sample type by clicking on the Task Column drop-down list:
  - a. NTC: target DNA detector task = **NTC**
  - b. NCS, test samples, and ERC wells: target DNA detector task = **Unknown**
2. Set up the standard curve as shown in table 7 and table 8:

Table 7. Settings for Hi5 Standard curve

Tube label	Task	Quantity (pg/ $\mu$ L)
ST1	Standard	30
ST2	Standard	3
ST3	Standard	0.3
ST4	Standard	0.03
ST5	Standard	0.003

Table 8. Settings for AcNPV Standard curve

Tube label	Task	Quantity (pg/µL)	Quantity (copies/µL)
ST1	Standard	$5.14 \times 10^5$	2
ST2	Standard	$5.14 \times 10^4$	0.2
ST3	Standard	$5.14 \times 10^3$	0.02
ST4	Standard	$5.14 \times 10^2$	0.002
ST5	Standard	$5.14 \times 10^1$	0.0002

3. Select the **Results** tab, then select Amplification Plot.
4. In the Data drop-down list, select **Delta Rn vs Cycle**.
5. In the Analysis Settings window, enter the following settings:
  - a. Select **Manual Ct**.
  - b. In the Threshold field, Hi5-DNA, AcNPV-DNA and IPC enter 0.02.
  - c. Select **Automatic Baseline**.
6. Click the button  in the toolbar, then wait the plate analyzing.
7. Select the **Result** tab> **Standard curve** tab, then verify the Slope, Intercept and R<sup>2</sup> values.
8. Select the Report tab, then achieve the mean quantity and standard deviation for each sample.
9. Select **File > Export > Results**. In the Save as type drop-down list, select **Results Export Files**, then click **Save**.

*Note: The parameter settings of the result analysis should be configured on the specific model and the software version, and generally can also be automatically interpreted by the instrument.*

10. In the Report Panel of Results, the 'Mean Quantity' column shows the detection values of NTC, NCS, test sample, in pg/µL or copies/µL.
11. The CT-IPC value of the sample and the CT-IPC value of the NCS should be within the range of  $\pm 1.0$  Ct value. If the Ct-IPC value of the sample is significantly higher than the Ct-IPC value of the NCS, it indicates that the sample may be inhibited. If the samples that include spiked reference standard

are tested at the same time, please consider the sample recovery rate as priority and take the IPC results as reference.

12. The Ct value of NCS should be larger than the mean Ct value of the lowest concentration in the standard curve, and shows normal amplification curve in the VIC signal channel. If the validated limit of quantitation (LOQ) concentration is less than the lowest concentration in the standard curve, the value of the NCS should be less than the concentration of LOQ.
13. The Ct value of NTC should be no less than 35.00 or undetermined, meanwhile shows normal amplification curve in the VIC signal channel.

Effective date: 01 Jul. 2024

## Support & Contact

**SHENTEK**

Biofargo, Inc.

[www.biofargo.com](http://www.biofargo.com)

Address: 1716 E Parham Rd Richmond, Va, 23228, USA

E-mail: [contact@biofargo.com](mailto:contact@biofargo.com)

Phone: 804-529-2296